

31 MAR 2005

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
15 April 2004 (15.04.2004)

PCT

(10) International Publication Number
WO 2004/031793 A1

(51) International Patent Classification⁷: **G01R 33/561**

Johan, S. [NL/NL]; c/o Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).

(21) International Application Number:
PCT/IB2003/004014

(74) Agent: **COHEN, Julius, S.**; Philips Intellectual Property & Standards, Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).

(22) International Filing Date:
12 September 2003 (12.09.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
02079089.5 1 October 2002 (01.10.2002) EP

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(71) Applicant (*for all designated States except US*): **KONINKLIJKE PHILIPS ELECTRONICS N.V.** [NL/NL]; Groenewoudseweg 1, NL-5621 BA Eindhoven (NL).


(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO,

(72) Inventor; and

(75) Inventor/Applicant (*for US only*): **VAN DEN BRINK,**

[Continued on next page]

(54) Title: A METHOD FOR K-SPACE DATA ACQUISITION AND MRI DEVICE

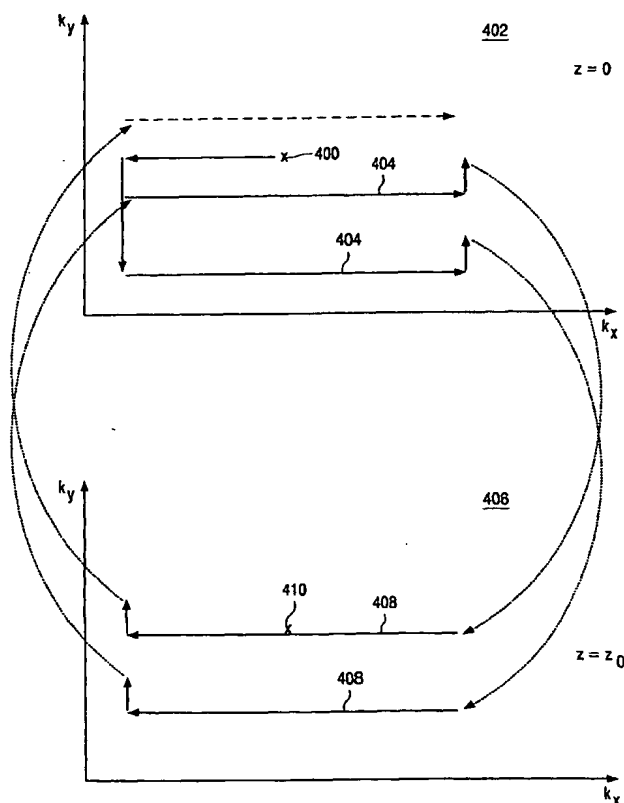

(57) Abstract: The invention relates to a method for interleaved k-space data acquisition for magnetic resonance imaging (MRI), the k-spaces having a first coordinate axis and a second coordinate axis, the method comprising: a) sampling into a first direction along the first coordinate axis, b) applying a first compensation pulse, c) sampling into a second direction along the first coordinate axis, the second direction being opposite to the first direction, applying a second compensation pulse, d) repetitively carrying out the steps a) to d).

WO 2004/031793 A1



SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG)

Declaration under Rule 4.17:

- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii)) for the following designations AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VC, VN, YU, ZA, ZM, ZW, ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU,

Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

A method for k-space data acquisition and MRI device

FIELD OF THE INVENTION

The present invention is related to the field of magnetic resonance imaging (MRI), and more particularly, to k-space data acquisition.

5 BACKGROUND AND PRIOR ART

The k-space notation is widely used in the art of MRI to establish a connection between spatial encoding (phase encoding and frequency encoding in the time domain) and the corresponding image obtained by applying the Fourier transform. For data acquisition in the k-space a sampling trajectory of a frequency-encoded signal is typically used. The basic
10 concepts of the k-space notation are explained in more detail in "Principles of Magnetic Resonance Imaging, a Signal Processing Perspective", Zhi-Pei Liang, Paul C. Lauterbur, IEEE Press Series in Biomedical Engineering, 2000, in particular chapter 5.2.3, pp. 157.

From P. Mansfield, "Multi-planar image formation using NMR spin echoes," J. Phys. C: Solid State Phys., vol. 10, pp. L55-L58, 1977 an MRI method is known which is
15 commonly referred to as echo-planar imaging (EPI). The term EPI is broadly used to refer to the class of high-speed imaging methods that collect a "complete" set of two dimensional encodings during the free induction decay period following a single excitation pulse. Hence, EPI has become a synonym for single-shot imaging, although multi shot EPI methods with interlaced k-space coverage are also in common use.

20 A key concept of EPI is the use of time-varying gradients to traverse k-space. For k-space data acquisition a variety of trajectories are known from the prior art such as zig-zag trajectory, rectilinear trajectory and spiral trajectory. For a discussion of the various prior art trajectories reference is made to the above referenced book of Liang and Lauterbur, chapter 9.3, pp. 303.

25 Figure 1 and Figure 2 show rectilinear trajectories for k-space EPI data acquisition.

In a first data acquisition step a first partial data acquisition of the k-space of the target region is obtained by following the trajectory as depicted in Figure 1. The trajectory starts at the central point 100 of the k-space. From there it goes into the lower left

corner 102 of the k-space. Starting from the lower left corner the k-space is partially scanned by means of a rectilinear trajectory. As it is known from WO 02 / 35 250 A1 half of the k-space is covered plus an additional seven lines.

5 After the first partial k-space acquisition in accordance with Figure 1 a brief z-shimming gradient pulse $z = z_0$ is applied before the second partial k-space data acquisition is performed in accordance with the trajectory of Figure 2.

The trajectory of Figure 2 is also rectilinear and starts at the point in k-space where the trajectory of the partial k-space acquisition of Figure 1 ends.

10 A k-space acquisition scheme of the type shown in Figures 1 and 2 is known from WO 02 / 35 250 A1 and from "Single-Shot EPI With Signal Recovery From the Susceptibility-Induced Losses", Allen W. Song, Magnetic Resonance in Medicine 46:407-411 (2001) for application in functional magnetic resonance imaging (fMRI). Based on each of the partial k-space data acquisitions an image is obtained and the two images are overlapped in order to produce a resulting image.

15 It is an object of the present invention to provide for an improved method for k-space data acquisition in order to increase the spatial sensitivity of MRI.

SUMMARY OF THE INVENTION

20 The present invention provides a method, a MRI device and a computer program product featuring improved k-space data acquisition for increased spatial sensitivity of the acquired images.

The present invention is based on the discovery that a forward and subsequent reverse k-space acquisition (cf. Figure 1 and Figure 2) leads to brain activations as detected with fMRI in very different places in the target region. In particular this decreases the
25 localisation and sensitivity of the resulting images in the blood oxygenation level-dependent (BOLD) statistical analysis.

The present invention provides a method for k-space data acquisition which overcomes this disadvantage of the prior art. In essence, the data acquisition in at least two k-space is performed in parallel in an interleaved manner. For example after sampling into a
30 first direction in the first k-space a compensation pulse is applied. A sampling is performed in the second k-space in the opposite direction. In the next step another compensation pulse is applied before the first k-space is again sampled in the first direction. The at least two k-spaces cover the same physical region, such as a slice of a patient's body. Individual images, each having its own information content, are associated with their respective k-spaces.

Within the framework of the present application the term compensation pulse indicates a pulse which affects artefacts in the reconstructed image. In particular such compensation pulses affect susceptibility artefacts. Very good results as to compensation of susceptibility artefacts are obtained when magnetic gradient pulses, such as 2-skinned gradient pulses are employed as compensation pulses.

In accordance with a preferred embodiment of the invention an image is formed based on the data samples which have been acquired for each of the at least two k-spaces. The images are combined to form a resulting image which features improved localisation and sensitivity.

The invention is particularly advantageous in that the echo times (TEs) for the two or more k-spaces do only have a small difference of for example less than 1 msec. This compares to the prior art, especially the Song reference, where even in the case of partial k-space coverage of the two echoes, the TEs differ by some eight to ten milliseconds. This results in an amplitude difference of the echo signals which affects the quality of the composite image, for both Sum-of Squares (SSQ) or Maximum Intensity Projection (MIP) combination. Typically, T2* (transverse relaxation time) being approximately 50 and 30 ms for main magnetic field strengths of 1.5T and 3T, respectively, the amplitude difference between the two images at an echo time difference of 10 ms will amount up to 30-40%, while BOLD related signal variations are typically on the order of 5-10%. Even amplitude correction will hamper adequate composite image formation in the prior art due to the image contrast mechanism of the BOLD effect.

As a consequence the small difference in the TEs which is accomplished in accordance with the invention has the effect to greatly enhance the quality of the composite image. This makes the invention particularly suitable for functional magnetic resonance imaging (fMRI).

It is a further advantage of the present invention that typical EPI corrections to line up echoes from positive and negative read out gradients do not need to be performed as all echoes contributing to one image have the same polarity. This improves the robustness of the IQ per "echo" image.

In accordance with a further preferred embodiment of the invention a larger number of k-spaces is utilized for the data acquisition. An even number of k-spaces is preferred as this has the advantage of not having to use the EPI phase correction when acquiring in both directions. Further it is preferred to apply a k_y gradient pulse after each

horizontal scan or after every n -th scan when a number of n of k -spaces with n different compensation values is used.

In accordance with a further preferred embodiment of the invention the TE difference for the two k -space data acquisitions is just the time of one horizontal readout
5 along the k_x axis.

As any k_y line for echo 1 is acquired immediately (one echo spacing, typically 0.5 - 0.8 ms) prior to the same line for echo 2, the result is that $k_y = 0$ (i.e. TE) for two "echo images" is just a single echo spacing apart. Consequently, the contrast (amplitude) of the images is the same, and combined usage of SSQ or MIP works much better in comparison to
10 the Song method.

In accordance with a further preferred embodiment of the invention the echo images are acquired with a partial Fourier coverage methodology. In particular the prior art problems with differing flow sensitivities in backward and forward partial Fourier EPI readouts can be resolved by application of the disclosed method.

15 In accordance with a further preferred embodiment of the invention the starting point for the sampling is the center of the k -space. From there the trajectory goes to the lower left corner of the first k -space. The following scans in the first k -space always go into the same direction. After each sampling along the k_x axis of the first k -space a compensation pulse such as a z -shimming pulse is applied before a sampling into the
20 opposite direction is performed for the second k -space. This way data acquisition for the two k -spaces is performed concurrently in an interleaved manner.

In accordance with a further preferred embodiment of the invention the k_y position of the sampling is incremented after each sampling along the horizontal axis in k_x or in $-k_x$ direction. Alternatively the k_y position is incremented only after sampling into the k_x or
25 $-k_x$ direction. In any case a compensation pulse is applied after each horizontal sampling in the k_x and $-k_x$ directions for the interleaved data acquisition.

In accordance with a further preferred embodiment of the invention the k -space data acquisition is performed partially for both k -spaces. This means that the combined trajectories of the k -space data acquisition cover half the k -space plus an additional couple of
30 lines. This way the read out time is reduced.

A further substantial advantage of the proposed method is that it enables to solve the problem of combining backward and forward partial fourier. This allows a shorter echo time, and it makes the functional contrast equal, especially by removing the difference in flow sensitivity.

In accordance with a further preferred embodiment of the invention the method of the invention is implemented in a computer program product. The computer program product can be used for the control unit of an MRI device in order to perform a method of the invention.

5

BRIEF DESCRIPTION OF THE DRAWINGS

In the following preferred embodiments of the invention will be described in greater detail by making reference to the drawings in which:

Figure 1 is a prior art example for partial k-space data acquisition,

10

Figure 2 is a prior art example for partial k-space data acquisition which is subsequent to the data acquisition of Figure 1 after application of a compensation pulse,

Figure 3 shows a MR devices having a control unit being programmed in accordance with an embodiment of a method of the invention,

Figure 4 is illustrative of an embodiment of a k-space data acquisition method in accordance with the invention,

15

Figure 5 is illustrative of a gradient switching diagram for the k-space data acquisition of Figure 4,

Figure 6 is illustrative of a flowchart for k-space data acquisition in accordance with the methods of Figures 4 or 5,

20

Figure 7 is illustrative of an embodiment of a k-space data acquisition method where a k_y gradient pulse is applied after every second horizontal scan,

Figure 8 is illustrative of a gradient switching diagram in accordance with the embodiment of Figure 7 of the inventive method,

Figure 9 is illustrative of an embodiment of a k-space data acquisition method with a number of $n = 4$ k-spaces,

25

Figure 10 is illustrative of a gradient switching diagram in accordance with the k-space data acquisition method of Figure 9.

DETAILED DESCRIPTION

30

Figure 3 shows a magnetic resonance device 1 which includes a first magnet system 2 for generating a steady magnetic field, and also several gradient coils 3 for generating additional magnetic fields having a gradient in the X, Y, Z directions. The Z direction of the co-ordinate system shown corresponds to the direction of the steady magnetic field in the magnet system 2 by convention. The measuring co-ordinate system x, y, z to be

used can be chosen independently of the X, Y, Z system shown in FIG. 3. The gradient coils are fed by a power supply unit 4. An RF transmitter coil 5 serves to generate RF magnetic fields and is connected to an RF transmitter and modulator 6.

5 A receiver coil is used to receive the magnetic resonance signal generated by the RF field in the object 7 to be examined, for example a human or animal body. This coil may be the same coil as the RF transmitter coil 5. Furthermore, the magnet system 2 encloses an examination space which is large enough to accommodate a part of the body 7 to be examined. The RF coil 5 is arranged around or on the part of the body 7 to be examined in this examination space. The RF transmitter coil 5 is connected to a signal amplifier and
10 demodulation unit 10 via a transmission/reception circuit 9.

The control unit 11 controls the RF transmitter and modulator 6 and the power supply unit 4 so as to generate special pulse sequences which contain RF pulses and gradients. The phase and amplitude obtained from the demodulation unit 10 are applied to a processing unit 12. The processing unit 12 processes the presented signal values (also
15 referred to as k-space) so as to form an image by transformation. This image can be visualized, for example by means of a monitor 13.

Figure 4 is illustrative of a method for k-space data acquisition in accordance with the invention. The starting point for the k-space data acquisition is the central point 400 of the k-space 402. From central point 400 the trajectory goes to the left in the $-k_x$ direction
20 and then to the lower left corner of the k-space 402 in the $-k_y$ direction.

Taking the lower left corner of the k-space 402 as a starting point a sampling 404 is performed in the k_x direction. After that the k_y position is incremented by applying a corresponding gradient pulse. Further a compensation pulse such as a z-shimming pulse is applied.

25 This way the trajectory continues in the k-space 406 where a sampling 408 is performed in the $-k_x$ direction. After the sampling 408 the k_y position is further increased by applying a further gradient pulse and another compensation pulse is applied such that the trajectory continues in the k-space 402.

In k-space 402 another sampling 404 is performed in the k_x direction. After
30 that again the k_y position is incremented and a compensation pulse is applied. As a consequence the trajectory continues in the k-space 406 where another sampling 408 is performed in the $-k_x$ direction etc. By continuing this operation of alternately sampling the k-spaces 402 and 406 k-space data acquisition is performed for both k-spaces 402 and 406 concurrently.

The resulting k-spaces 402 and 406 have both been undersampled with alternating k_y -lines being acquired. This results in aliased images, which can be 'unfolded' using a multiple receiver coil set-up and known coil sensitivity profiles, i.e. by applying parallel imaging, e.g. the SENSE or the SMASH method, or its hybrids and variants.

5 Preferably the k-space data acquisition is performed only partially for the k-spaces 402 and 406 in order to reduce the read-out time.

It is to be noted that the TE is about the same for both k-spaces 402 and 406 when TE is defined as the time from the start of the data acquisition to the time when the central point 400 of the k-space 402 and central point 410 of the k-space 406 are reached by
10 the trajectory. This way the contrast resolution of the resulting image is increased.

Rather than applying a gradient pulse after each horizontal scan to increase the k_y position this can also be done only after every second scan. For example after sampling 404 has been performed no gradient pulse is applied in order to increase the k_y position. Rather only a compensation pulse is applied before sampling 408 is carried out on the same
15 k_y position. After sampling 408 the k_y position is incremented by means of a corresponding gradient pulse.

Further it is important to note that the gradient pulse to increase the k_y position and the compensation pulse can be applied concurrently.

Figure 5 shows a diagram of the gradient channel signals for the embodiment
20 of Figure 4 where the k_y position is incremented after every horizontal scan.

The signal G_x is illustrative of the horizontal gradient pulses which are applied for horizontal sampling along the k_x or $-k_x$ axis. The signal G_x has negative pulses e1 and positive pulses e2. The signal G_x is constituted by an alternating sequence of negative pulses e1 and positive pulses e2. For example a negative pulse e1 corresponds to one sampling into
25 the k_x direction (cf. sampling 404 of Figure 4) whereas a positive pulse e2 corresponds to a sampling into the opposite direction (cf. sampling 408 of Figure 4).

The signal G_y represents the gradient pulses which are applied for incrementing the k_y positions of the data samplings. A G_y pulse is applied after each e1 and after each e2 pulse in the embodiment considered here.

30 The signal G_z is illustrative of compensation pulses, such as z-shimming compensation pulses, which are applied during the data acquisition in order to "switch" between the two k-spaces (cf. k-spaces 402 and 406 of Figure 4). A compensation pulse is applied after each signal e1 or e2.

It is important to note, that the k-space lines for the two images obtained are sampled in an interleaved manner, and that as a consequence, all read-outs for one of the k-spaces have the same sign. This is advantageous in EPI reconstruction of the individual images (cf. steps 514 and 516) as no phase correction is needed. The final image is obtained as a SSQ or MIP of the two images of the two k-spaces. For the image construction it is a particular advantage that the echo times are equal with only one echo spacing difference.

Figure 6 is illustrative of a corresponding flow diagram.

In step 500 data acquisition is performed into the k_x direction of the first k-space. In step 502 the k_y position for the sampling is incremented by applying a corresponding gradient pulse. In step 504 a z-shimming pulse is applied which brings the trajectory into the other k-space.

In the other k-space a sampling is performed into the opposite $-k_x$ direction. In step 508 k_y is again incremented and another z-shimming pulse is applied in step 510 which brings the trajectory back into the first k-space.

In step 512 another sampling is performed into the k_x direction. This procedure continues until a sufficient amount of data samples for the two k-spaces has been obtained for image generation.

In step 514 a first image is generated based on the data samples acquired in the first k-space by sampling into the k_x direction. Likewise in step 516 a second image is generated based on the data samples acquired in the other k-space by sampling into the opposite direction.

In step 520 the two images of steps 514 and 516 are combined to provide the resulting image.

In essence, Figures 5 and 6 are descriptive of a method which employs a parallel imaging reduction factor of 2, and 2 z-shim values: echoes for the first and second image are sampled alternately, and consecutively blips along G_y move to the next k_y line while moving to the next k-space. As such, each individual k-space is undersampled by a factor of 2. The reconstruction of the corresponding aliased images is performed using the known coil sensitivities according to e.g. the SENSE or the SMASH methodology. The z-shim gradient is applied between the echoes for the first and second image, and rewound before acquiring the next k_y position echo for the first image.

Figure 7 is illustrative of an alternative method for a k-space data acquisition. The same reference numerals are used in Figure 7 as in Figure 4 in order to designate like

elements. In contrast to the embodiment of Figure 4 a k_y gradient pulse is applied only after every second horizontal scan in the k-space 406.

Figure 8 shows a diagram of the representative gradient channel signals for the preferred embodiment where the k_y position is incremented after every second horizontal scan. In the embodiment considered here a G_y pulse is applied after each pair of $e1$ and $e2$ pulses.

Figure 9 is illustrative of an embodiment where an interleaved k-space data acquisition scheme is used which involves a number of $n = 4$ k-spaces. Figure 10 shows the corresponding gradient channel signals. The echoes for the first to the forth image are sampled alternately, and consecutive blips along G_y move to the next k_y line while moving to the next k-space. The z-shim gradient is applied between the echoes for the first, second, third and forth image, and rewind before acquiring the next k_y position echo for the first image. This way a parallel imaging reduction factor r of $r=n=4$ is accomplished.

LIST OF REFERENCE NUMERALS

	magnetic resonance device	1
	magnet system	2
5	gradient coil	3
	supply unit	4
	transmitter coil	5
	modulator	6
	object	7
10	transmission / reception circuit	9
	demodulation unit	10
	control unit	11
	processing unit	12
	monitor	13
15	central point	100
	corner	102
	central point	400
	k-space	402
	sampling	404
20	k-space	406
	sampling	408
	central point	410

CLAIMS:

1. A method for k-space data acquisition for magnetic resonance imaging (MRI) characterized by using of at least first and second k-spaces for interleaved data acquisition, the at least first and second k-spaces covering substantially the same physical region.
- 5 2. The method of claim 1, the k-spaces having a first coordinate axis and a second coordinate axis, the method comprising:
 - a) sampling into a first direction along the first coordinate axis,
 - b) applying a first compensation pulse,
 - 10 c) sampling into a second direction along the first coordinate axis, the second direction being opposite to the first direction,
 - d) applying a second compensation pulse,
 - e) repetitively carrying out the steps a) to d).
- 15 3. The method of claims 1 or 2, the first and second compensation pulses being z-shimming pulses.
4. The method of claims 1, 2 or 3, further comprising incrementing a sampling position on the second coordinate axis after each step a) and / or after each step b).
- 20 5. The method of anyone of the preceding claims 1 to 4, further comprising performing a partial k-space data acquisition by means of the sampling in steps a) and c).
6. The method of anyone of the preceding claims 1 to 5 further comprising combining the sampled data of steps a) and c) to generate an image.
- 25 7. The method of anyone of the preceding claims 1 to 6 further comprising generating a first image based on the data samples being acquired in the first direction, generating a second image based on the data samples acquired in the second direction and combining the first and second images into one image.

8. The method of anyone of the proceeding claims 1 to 7, whereby a number of n k-spaces is used for the interleaved data acquisition, and further comprising the steps of:

- applying a number of $n-1$ first compensation pulses of a first amplitude,
- 5 - applying the second compensation pulse with a second amplitude, where the second amplitude is $n-1$ times the first amplitude.

9. A magnetic resonance imaging (MRI) device comprising means for interleaved k-space data acquisition in at least first and second k-spaces.

10

10. The magnetic resonance imaging device of claim 9 comprising:

- means (2, 3, 4, 5, 6, 9, 10) for k-space data acquisition, the k-spaces having a first coordinate axis and a second coordinate axis,
- a control unit (11) for generating of control signals for the means for k-space data
- 15 acquisition,

wherein the control signals cause the means for k-space data acquisition to

- a) sample into a first direction along the first coordinate axis,
- b) apply a first compensation pulse,
- c) sample into a second direction along the first coordinate axis, the second direction
- 20 being opposite of the first direction,
- d) apply a second compensation pulse,
- e) repetitively carry out the steps a) to d).

11. A computer program product for k-space data acquisition for magnetic resonance imaging (MRI), the computer program product comprising program means to perform k-space data acquisition in at least first and second k-spaces in an interleaved way.

25

12. The computer program products of claim 11, the k-spaces having a first coordinate access, the program means being adapted to perform the steps of :

30

- a) sampling into a first direction along the first coordinate axis,
- b) applying a first compensation pulse,
- c) sampling into a second direction along the first coordinate axis, the second direction being opposite to the first direction,
- d) applying a second compensation pulse,

e) repetitively carrying out the steps a) to d).

1/8

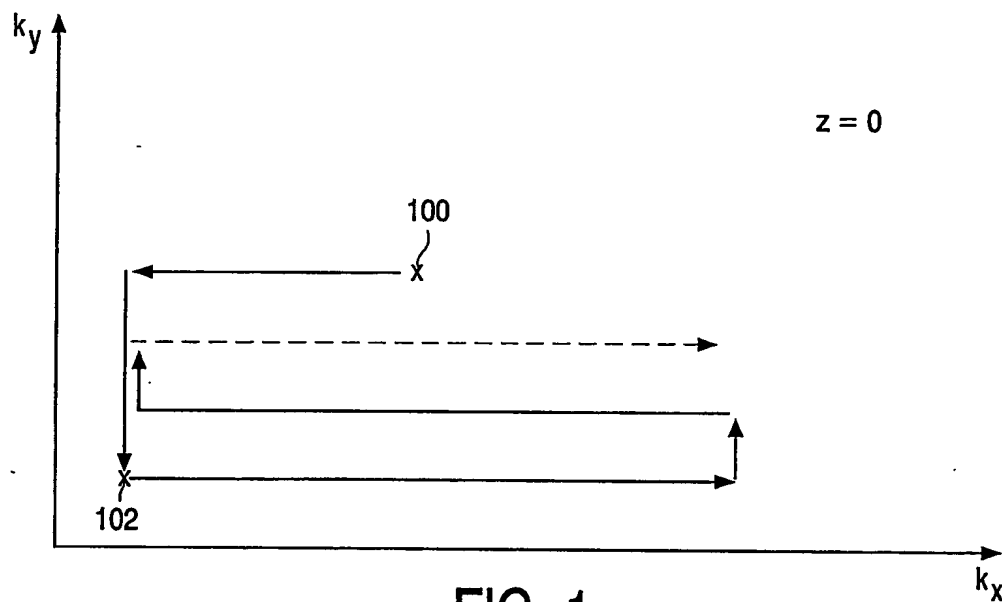


FIG. 1

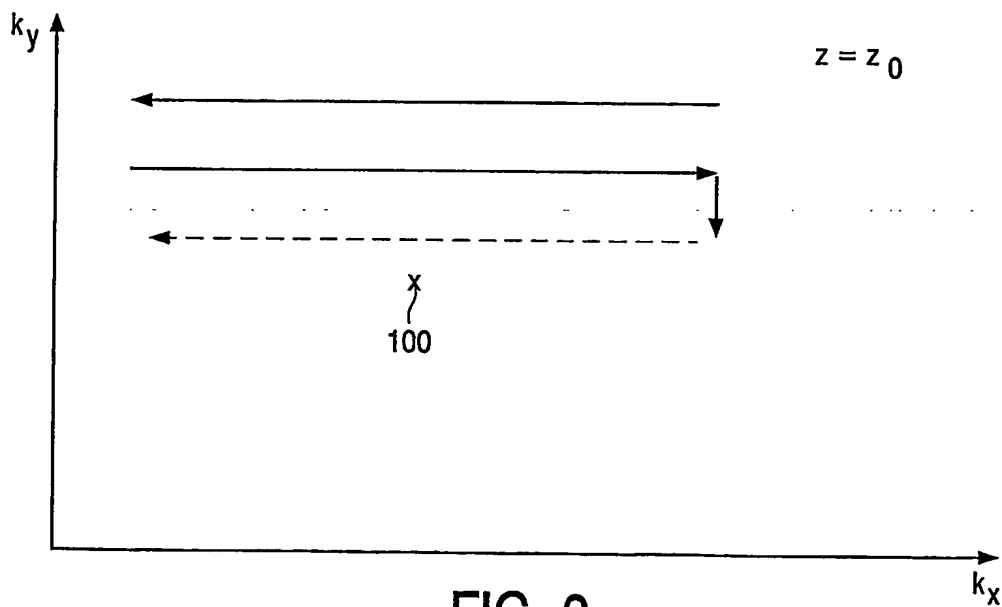


FIG. 2

2/8

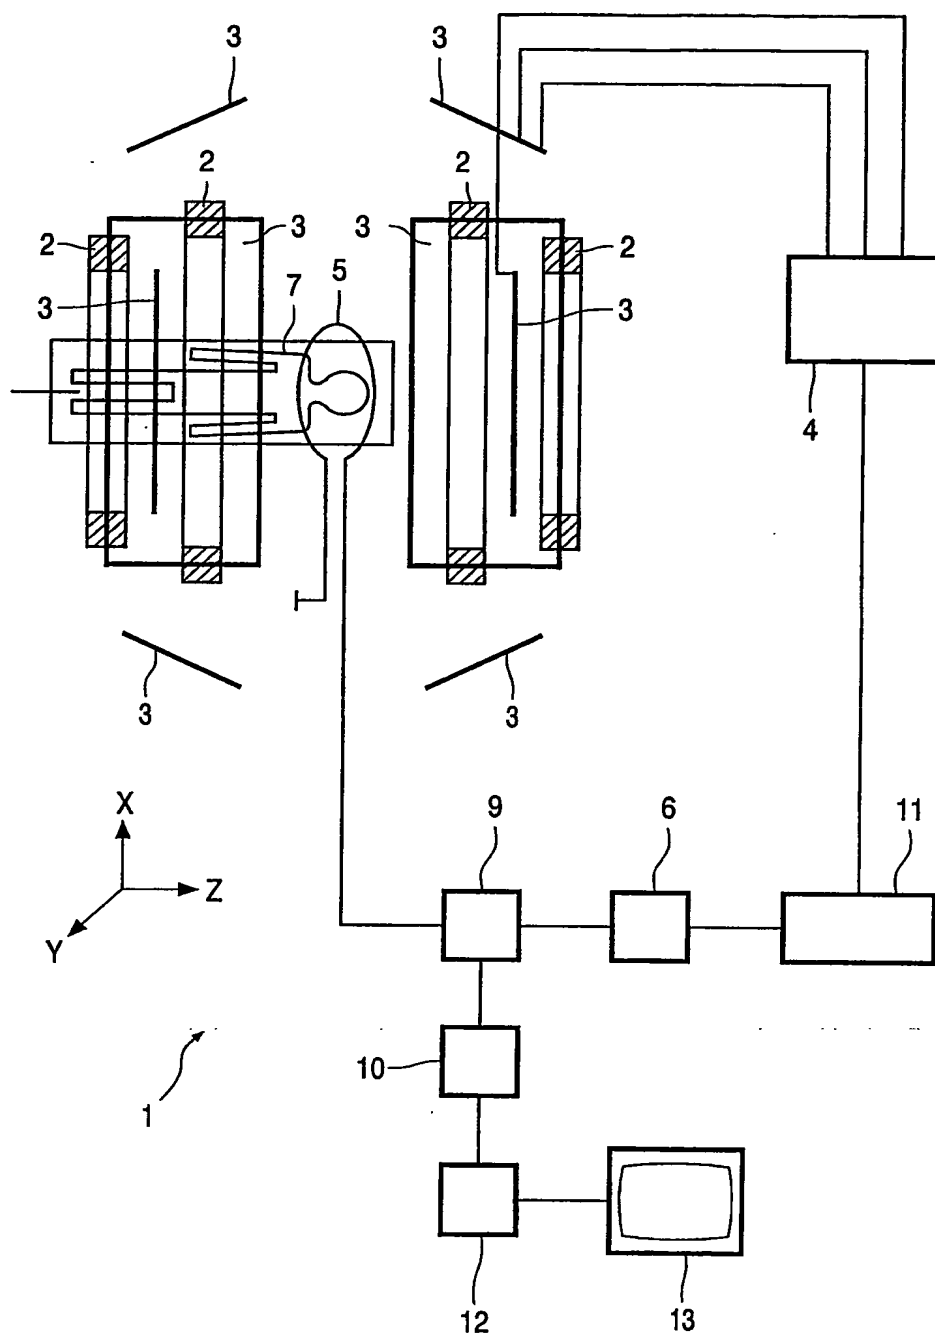


FIG. 3

3/8

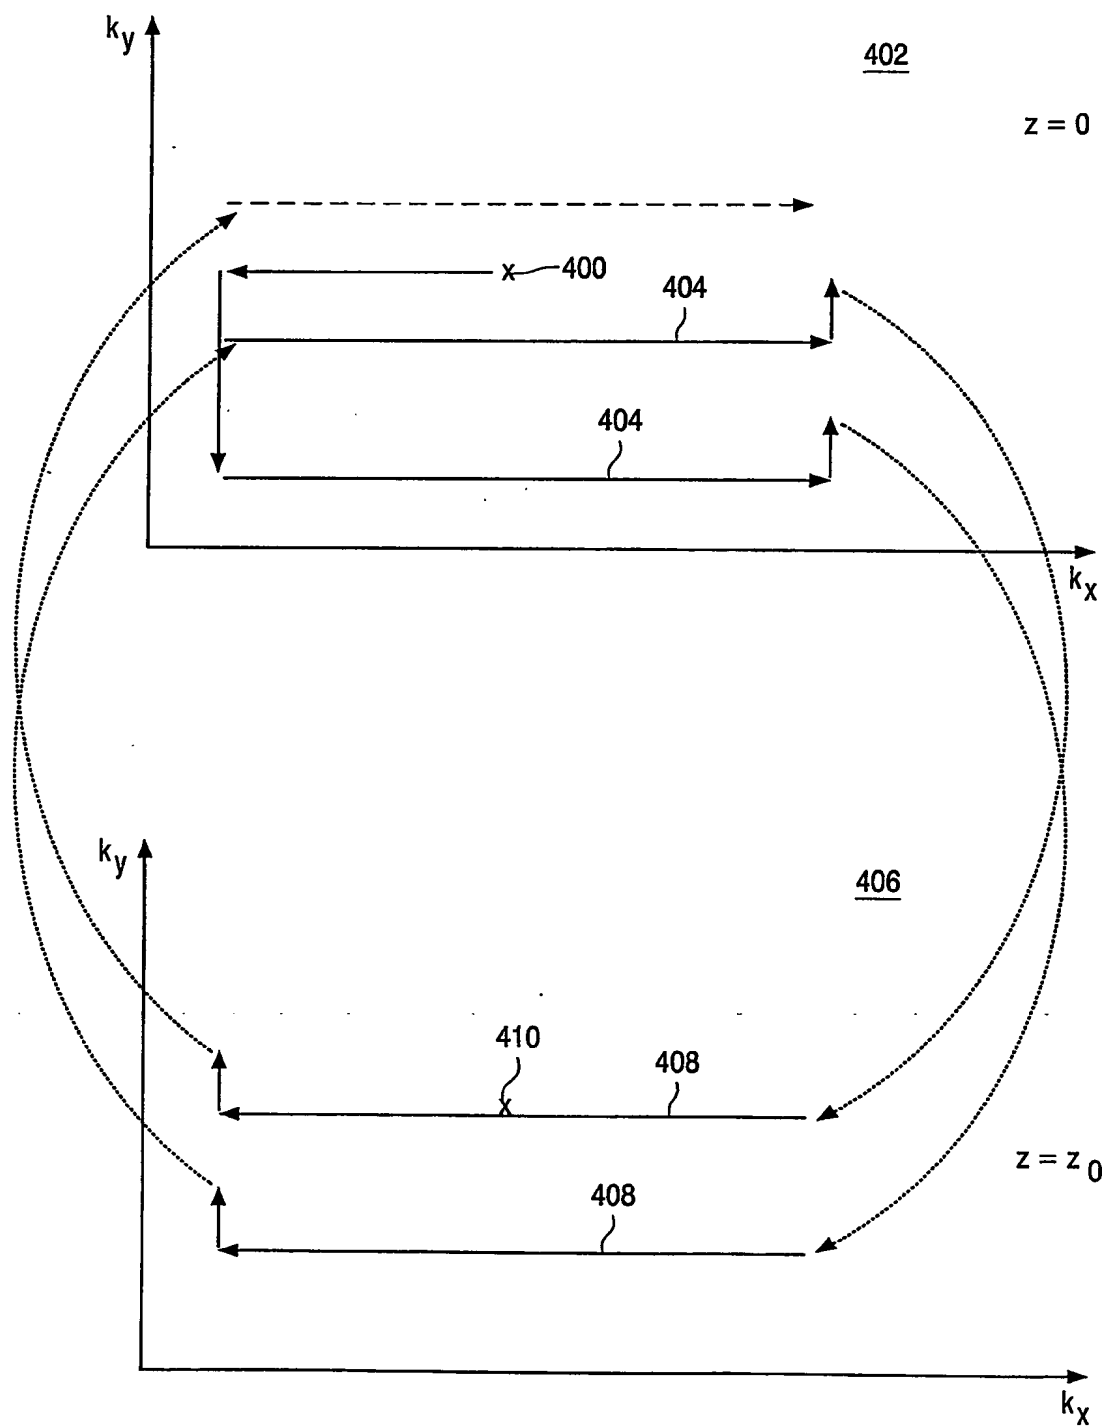


FIG. 4

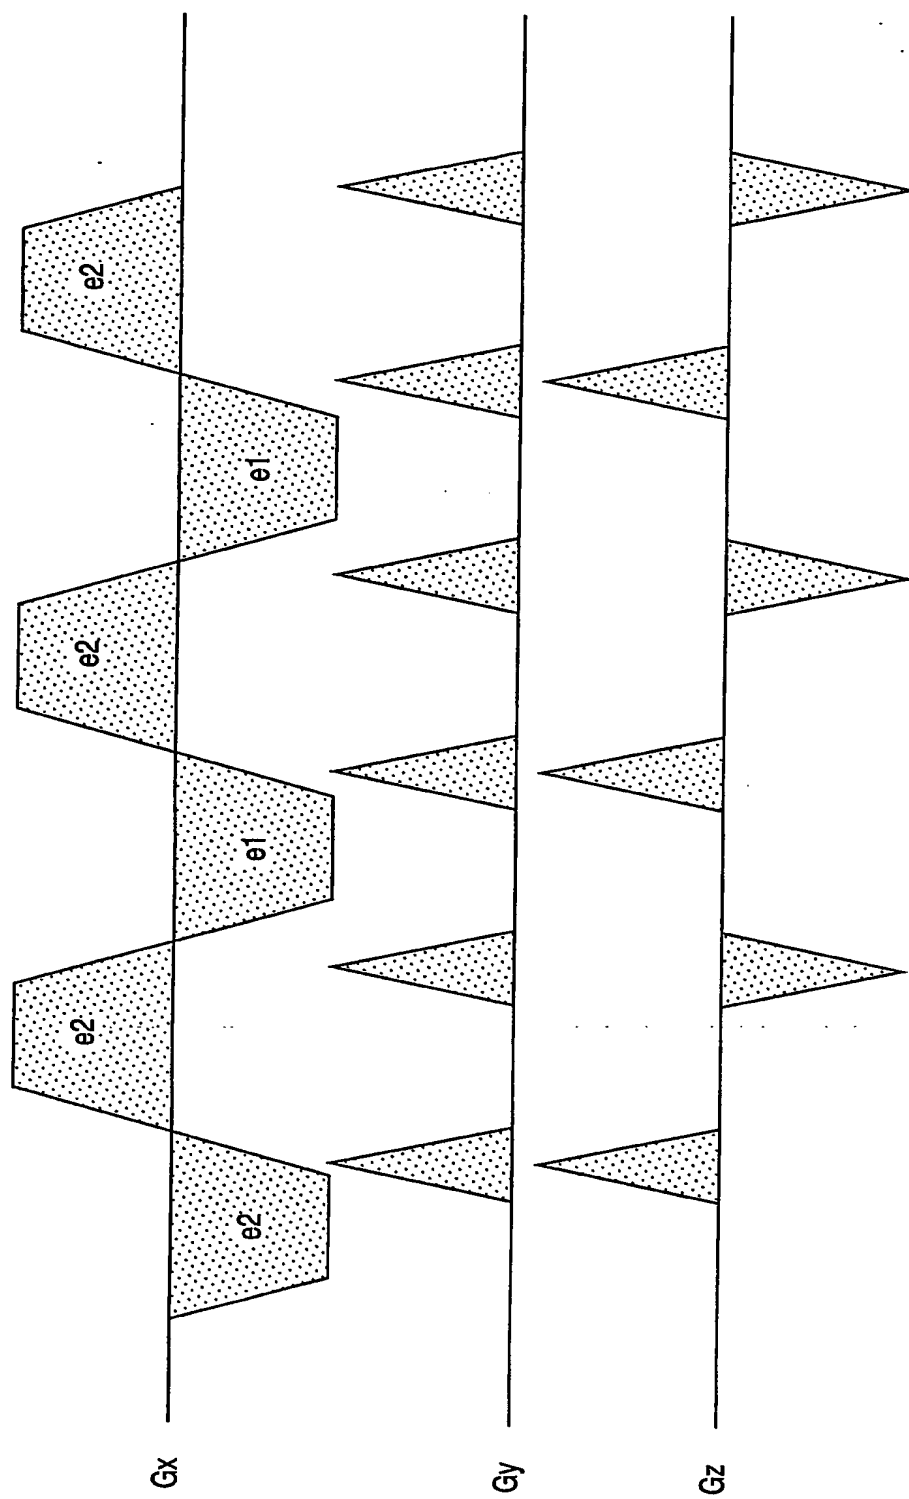


FIG. 5

5/8

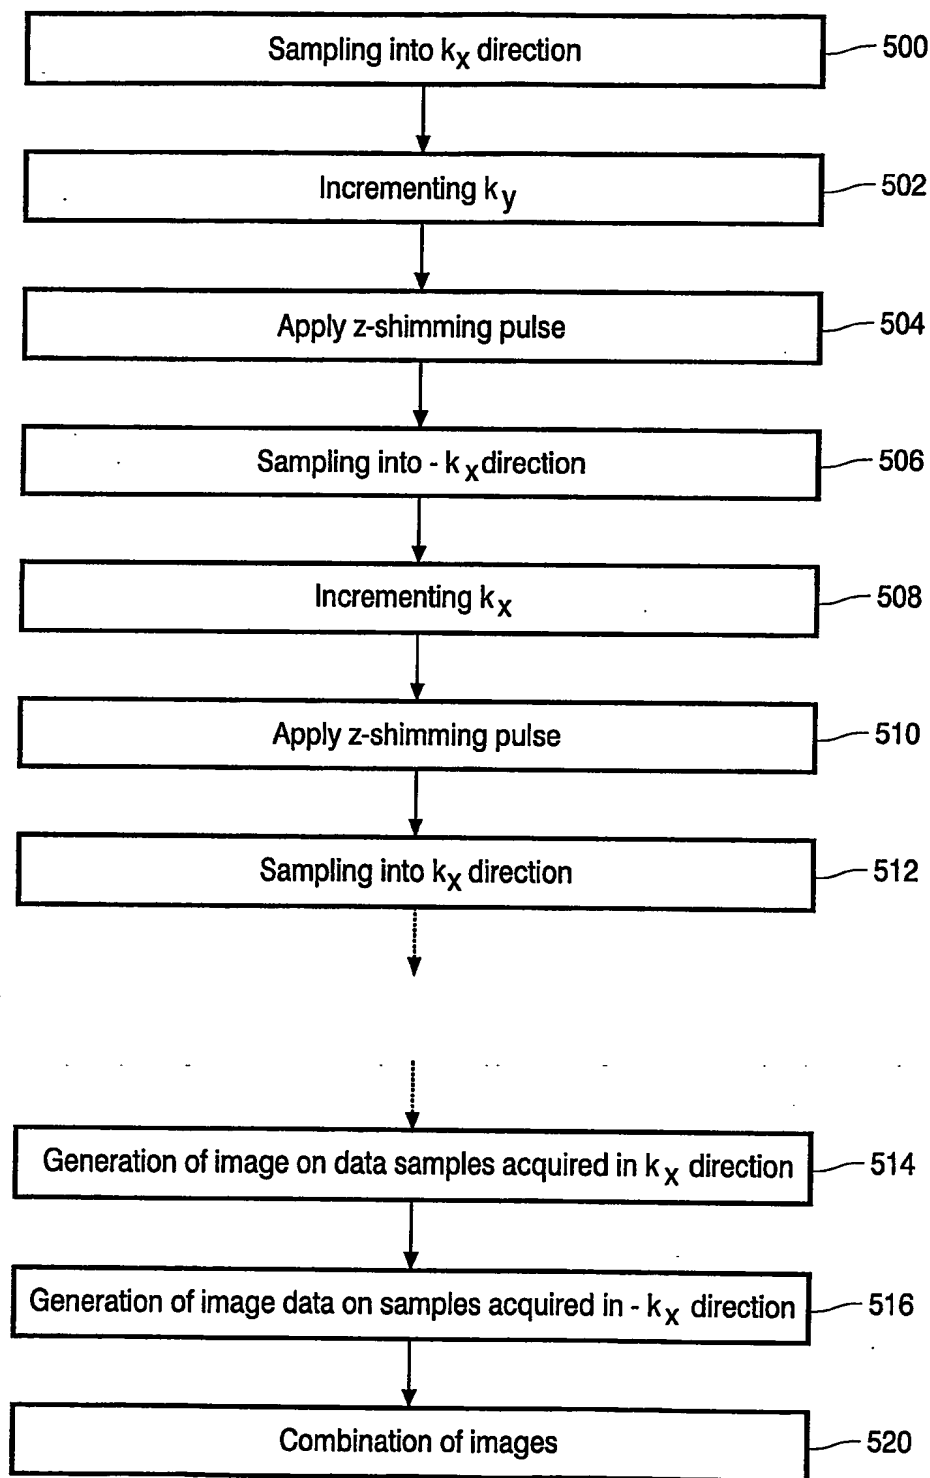


FIG. 6

6/8

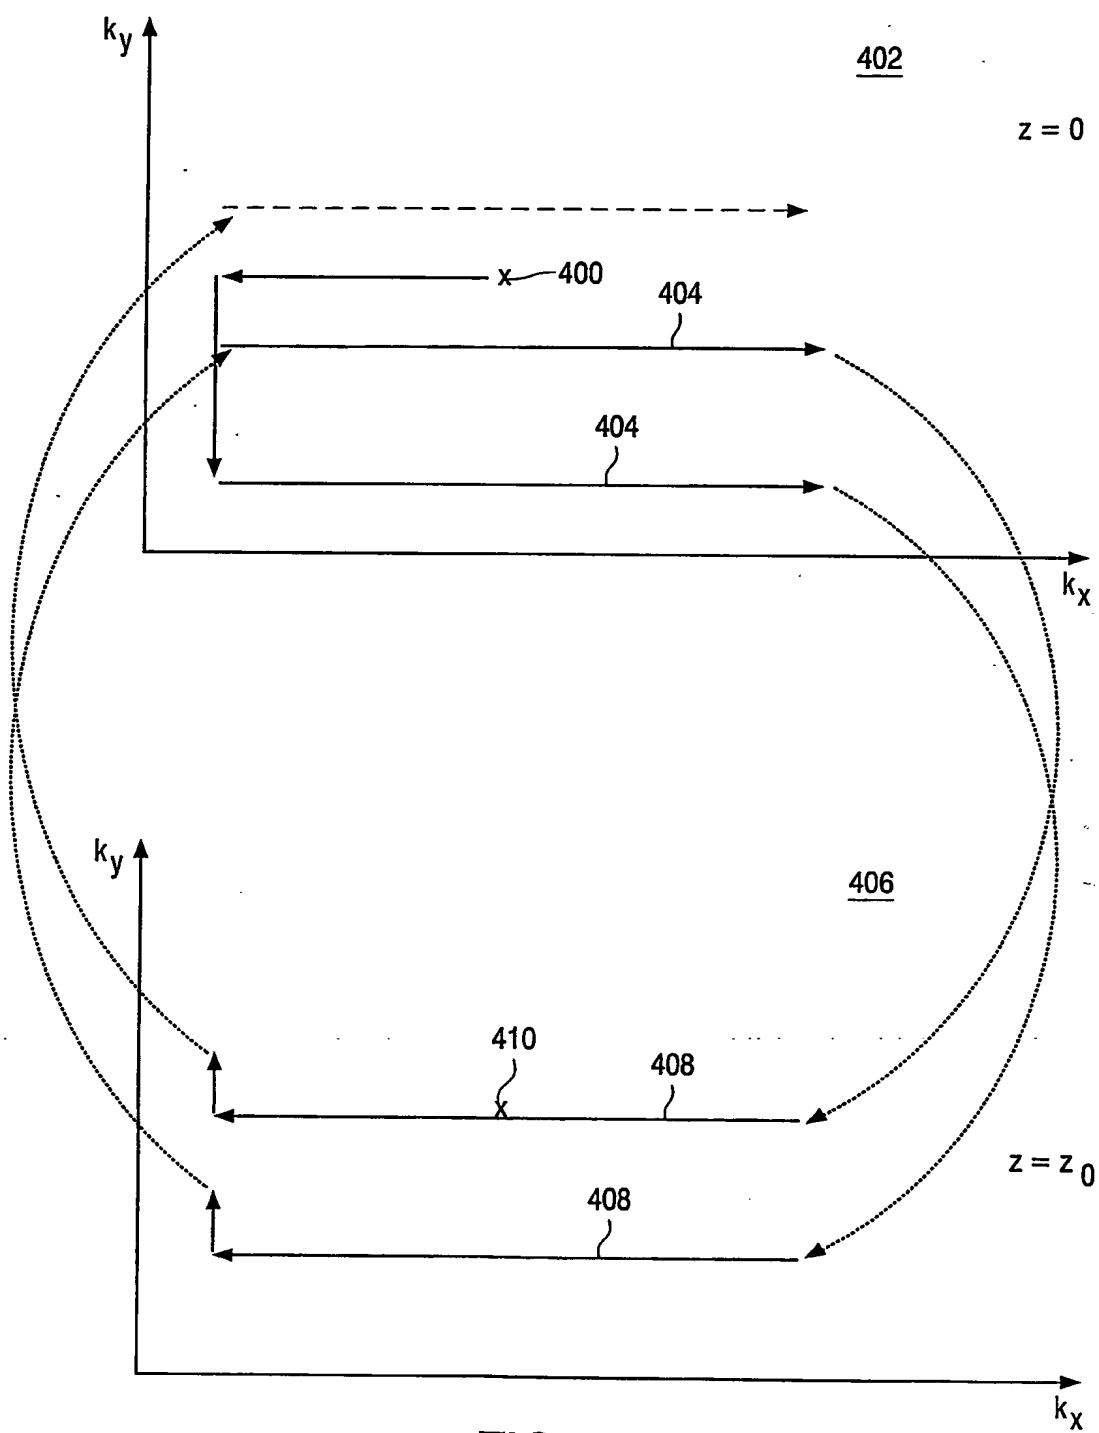


FIG. 7

7/8

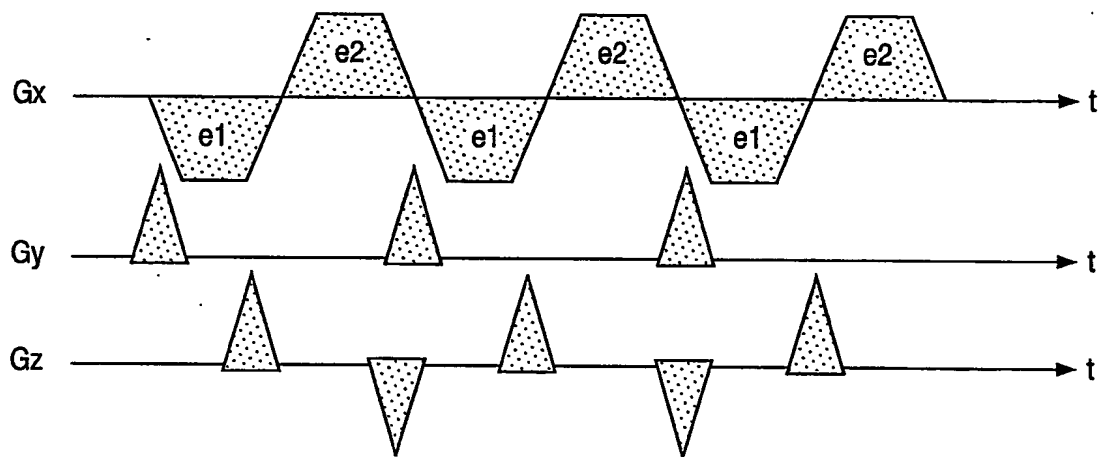


FIG. 8

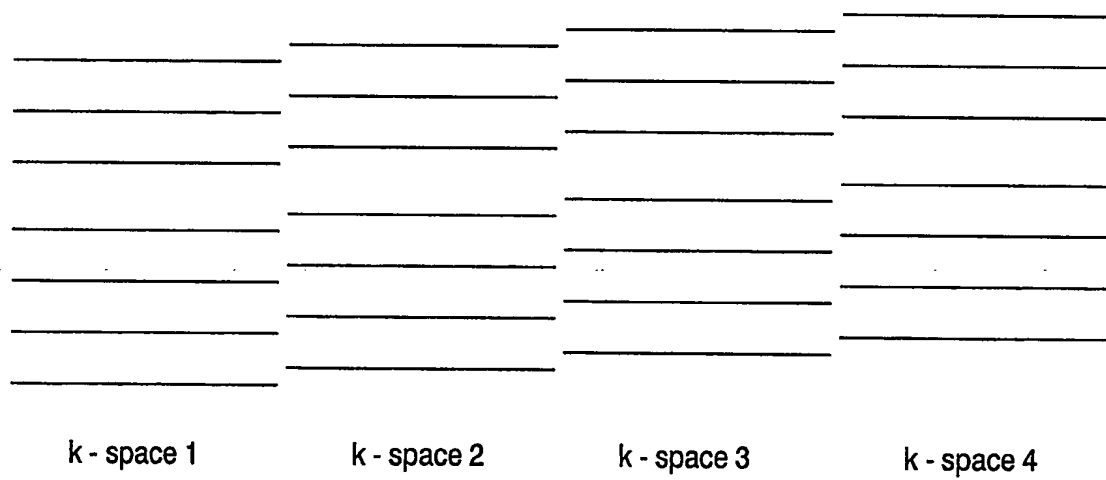


FIG. 9

8/8

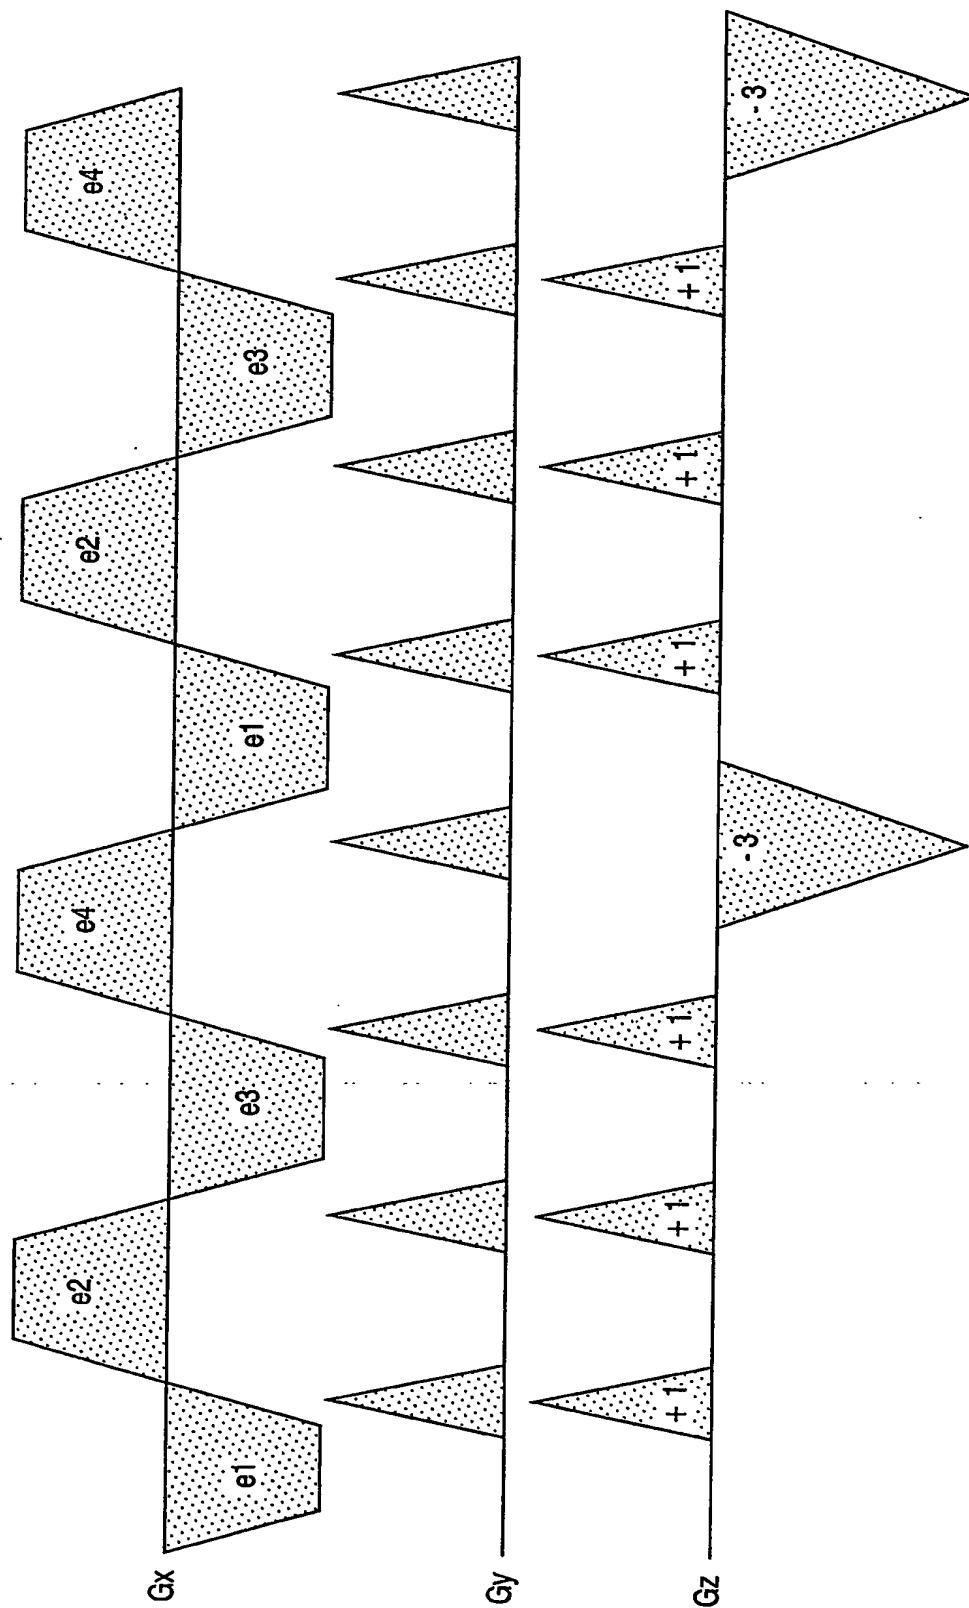


FIG. 10

INTERNATIONAL SEARCH REPORT

Int. Patent Application No.
PCT/JP03/04014

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 G01R33/561

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 G01R

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

INSPEC, MEDLINE, EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	M.H. BUONOCORE, D.C. ZHU: "High spatial resolution EPI using an odd number of interleaves" MAGNETIC RESONANCE IN MEDICINE, vol. 41, 1999, pages 1199-1205, XP000825803 ISSN: 0740-3194 pages 119 - the whole document	1,2,4-7, 9-12
X	G.T. LUK PAT ET AL.: "Reducing flow artifacts in echo-planar imaging." MAGNETIC RESONANCE IN MEDICINE, vol. 37, 1997, pages 436-447, XP000682117 ISSN: 0740-3194 pages 438 - 444: "READOUT PROPERTIES" - "IMPLEMENTATION"; Fig. 2 --/--	1,2,4-7, 9-12

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents:

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *&* document member of the same patent family

Date of the actual completion of the international search

20 February 2004

Date of mailing of the international search report

26/02/2004

Name and mailing address of the ISA
European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Volmer, W

INTERNATIONAL SEARCH REPORT

International Application No.

PCT/IB 03/04014

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 6 044 290 A (K.K. VIGEN ET AL.) 28 March 2000 (2000-03-28) column 4, line 218 - line 48 column 6, line 66 -column 9, line 9 figures 3-5	1,2,4-7, 9-12
X	WO 02 35250 A (DUKE UNIVERSITY) 2 May 2002 (2002-05-02) cited in the application	1,9,11
A	page 4, line 19 -page 6, line 7 page 10, line 4 -page 13, line 19 figure 3	2-8,10, 12
X	L.P. PANYCH ET AL.: "Selection of high-definition 2D virtual profiles with multiple RF pulse excitations along interleaved echo-planar k-space trajectories" MAGNETIC RESONANCE IN MEDICINE, ACADEMIC PRESS, DULUTH, MN, US, vol. 41, 1999, pages 224-229, XP002217965 ISSN: 0740-3194 pages 224 - 226: "METHODS"; Figs. 1, 2	1,9,11

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No
PCT/JP03/04014

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 6044290	A	28-03-2000	NONE	
WO 0235250	A	02-05-2002	AU 1326602 A	06-05-2002
			WO 0235250 A1	02-05-2002
			US 2002082497 A1	27-06-2002